


Setup

Conc Test

Temp Test

pH Test

Christian Alarapon

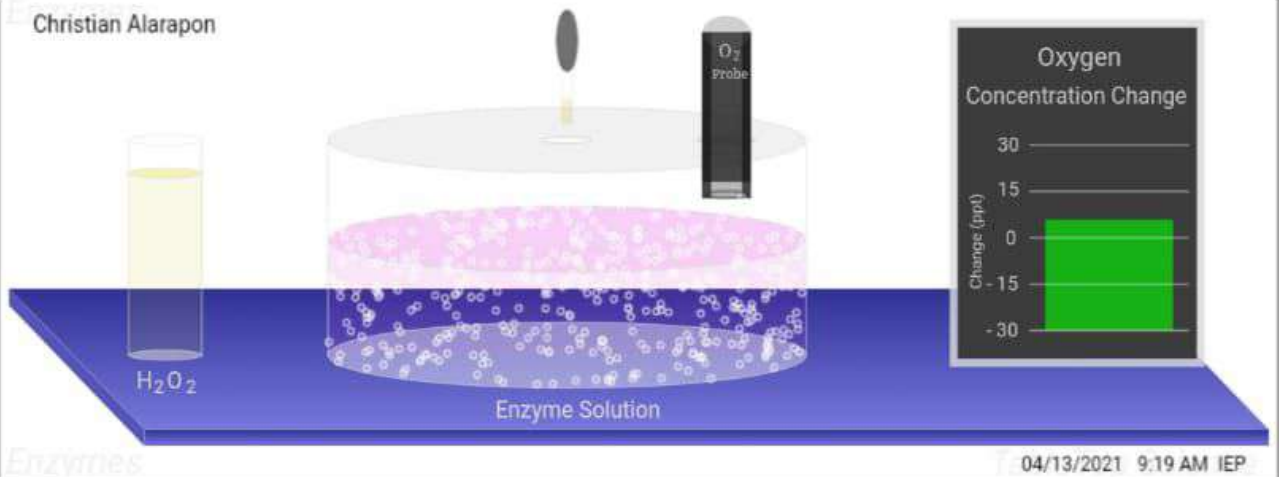

04/13/2021 9:19 AM IEP

Start Data Run

Concentration: 2.5 %

Temperature: 25.0 °C

pH: 7.0

Time: 20.0 s

Reset

concentration slider

Data Run Complete!

O₂ Change: 5.64 ppt